
Patterson DICOM Imaging

DICOM Conformance Statement

Notice

The software described in this document has been validated in accordance with the governing DICOM standard at the time of this document's release. Patterson Dental Supply, Inc. shall not be liable for errors contained herein or consequential damages in connection with the furnishing, performance, or use of this document.

Patterson Dental Supply, Inc. reserves the right to revise this publication and to make changes to its content at any time, without obligation to notify any person or entity of such revisions and changes.

Copyright © 2004 Patterson Dental Supply, Inc., Inc. All Rights Reserved



2202 Althoff Drive
P.O. Box 1267
Effingham, IL 62401
Corporate: 217.347.5964
Sales: 800.294.8504
Fax: 217.342.6950
www.eaglesoft.net

Contents

DICOM	1
Introduction	1
Implementation Model.....	3
Patterson Imaging AE Specifications	5
Communication Profiles	10
Configuration.....	10

DICOM

Introduction

1.1. Overview

This document is the DICOM Conformance Statement for Patterson DICOM Imaging, the image acquisition component of the client-server software applications Patterson EagleSoft and Patterson Imaging from Patterson Dental Supply, Inc. In its primary role, Patterson DICOM Imaging will request access, storage, and retrieval of images from a DICOM 3.0 conformant server.

1.2. Intended Audience

The reader of this document is concerned with software design and/or system integration issues. It is assumed that the reader of this document is familiar with the DICOM 3.0 Standard and the terminology and concepts employed in those documents.

Readers wishing to obtain more familiarity with the content and terminology of DICOM 3.0 Standard are encouraged to obtain and review the standard prior to reading this Conformance Statement. More information on acquiring this document and its updates on the DICOM standard may be found on the website of the National Electrical Manufacturer's Association (NEMA) at <http://www.nema.com>.

1.3. Scope and Field of Application

It is the intent of this document to describe the appropriate and decided communication of data between Patterson DICOM Imaging and a DICOM 3.0 conformant server application.

1.4. Important Remarks

The use of the Patterson DICOM Imaging Conformance Statement, in conjunction with DICOM 3.0 Standard, is intended to facilitate communication between Patterson software and other applications. These standards, by themselves, should not be the sole source for, or guarantee of, interoperability between Patterson software and other non-Patterson applications or equipment. Responsibility for

the correct design and integration of Patterson software within the framework of other systems remains with the user and should not be minimized or overlooked. Users are strongly urged to test and validate the proper interaction between Patterson and other non-Patterson applications or devices before declaring operability.

1.5. References

In preparing this conformance statement, frequent reference to the DICOM Standard, particularly PS 3.1 through PS 3.5, PS 3.7, PS 3.8, and PS 3.10 through PS 3.12 was made.

1.6. Acronyms

The following acronyms appear in this document and are defined below.

AE	Application Entity
CT	Computerized Tomography
CUID	Class Unique Identifier
DICOM	Digital Imaging and Communications in Medicine
MR	Magnetic Resonance
NEMA	National Electrical Manufacturers' Association
SCP	Service Class Provider
SCU	Service Class User
TCP/IP	Transmission Control Protocol / Internet Protocol
UID	Unique Identifier
VL	Visible Light

Implementation Model

2.1. Application Data Flow Diagram

The Patterson DICOM Imaging Application Entity (AE) is an application that initiates requests for the storage and retrieval of stored images and access to patient information. These requests originate with Patterson DICOM Imaging which interfaces with the server by DICOM association. The implementation model of the Patterson DICOM Imaging AE is shown in the following figure.

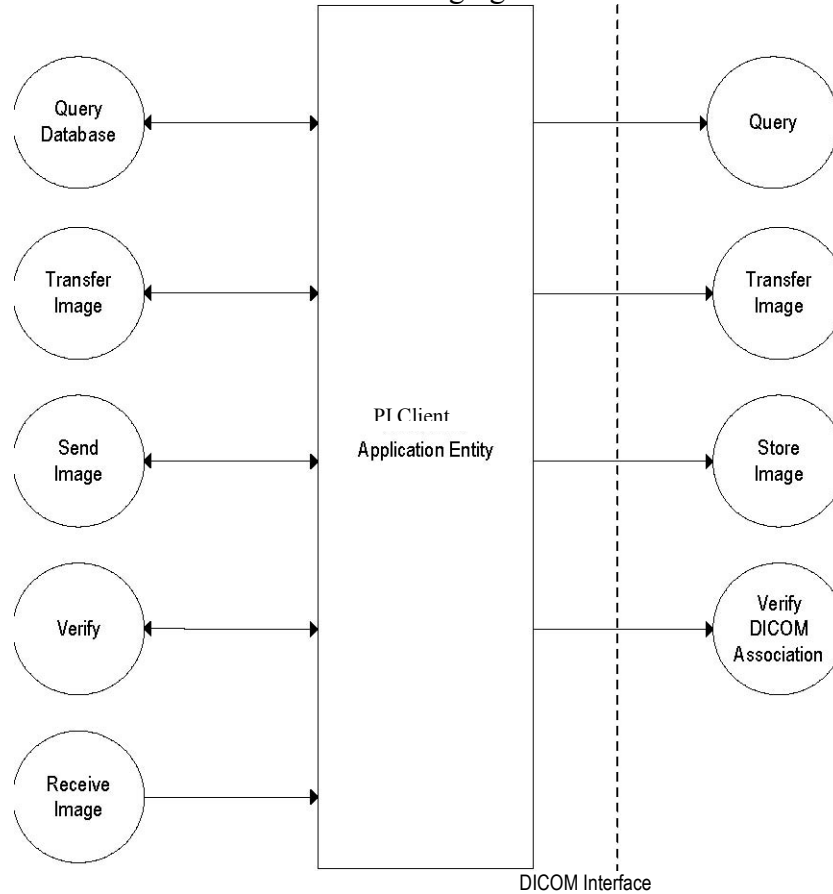


Figure 1. Implementation Model for Patterson DICOM Imaging Application Entity

2.2. Functional Definitions

The Patterson DICOM Imaging AE is an application initiating requests for image storage and retrieval from a DICOM 3.0 conformant server.

Patterson DICOM Imaging acts as a service class provider (SCP) in the following role:

1. SCP for C-Store operations to Storage service class users (during MOVE operations only)

Patterson DICOM Imaging acts as a service class user (SCU) in the following roles:

1. SCU of C-Store operations from Storage service class providers
2. SCU of C-Echo operations from Verification service class providers
3. SCU of C-Find operations from Query / Retrieve service class providers
4. SCU of C-Move operations from Query / Retrieve service class providers

2.2.1. Query Database

Patterson DICOM Imaging can initiate a request (C-Find-RQ) for patient, study, and image queries. Patterson DICOM Imaging provides in this request all the values for the attributes it wishes to match.

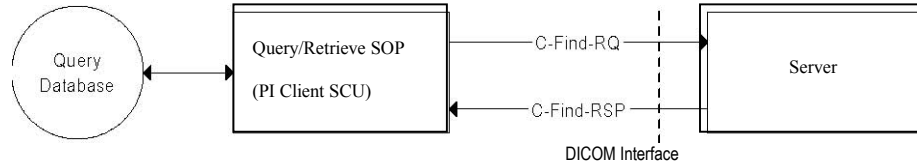


Figure 2. Query Database Model

2.2.2. Transfer Image

Patterson DICOM Imaging can initiate an image move request (C-Move-RQ) and supplies unique values that identify the move destination to the server (AE name, IP address, and port number). Patterson DICOM Imaging also receives a status message confirming the operation.

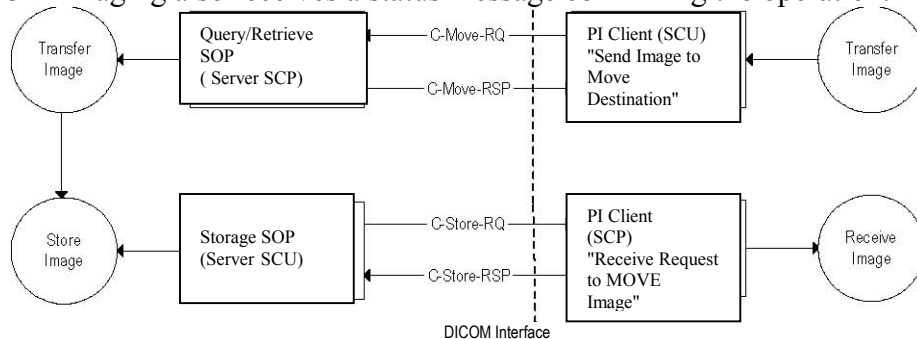


Figure 3. Transfer Image Model

2.2.3. Send and Store Image

Patterson DICOM Imaging can initiate a request (C-Store-RQ) to store images it has acquired. Patterson DICOM Imaging also receives a status message confirming the operation.

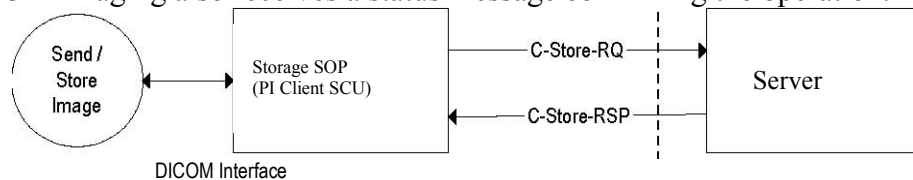


Figure 4. Send / Store Image Model

2.2.4. Verify

Patterson DICOM Imaging can initiate a request (C-Echo-RQ) to verify a current DICOM association.

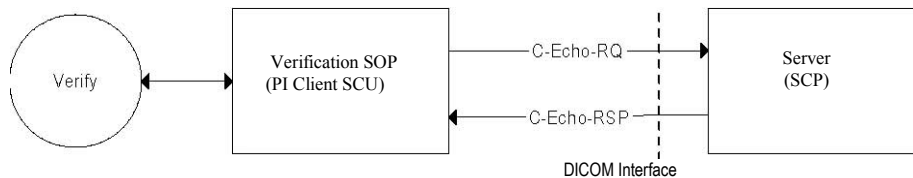


Figure 5. Verify Model

2.3. Sequencing of Real World Activities

Not applicable

Patterson Imaging AE Specifications

3.1. Patterson DICOM Imaging AE Specification

3.1.1. Storage - Specification

Patterson DICOM Imaging provides Standard Conformance to the following DICOM 3.0 Standard SOP Class as a SCU.

Table 1. Storage SOP Classes Supported by Patterson DICOM Imaging

SOP Class Name	SOP Class UID
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
CT Image Storage	1.2.840.10008.5.1.4.1.1.2
MR Image Storage	1.2.840.10008.5.1.4.1.1.4
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
Ultrasound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
X-ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Digital X-ray Image Storage for Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital X-ray Image Storage for Processing	1.2.840.10008.5.1.4.1.1.1.1.1
Digital Intra-oral X-ray Image Storage for Presentation	1.2.840.10008.5.1.4.1.1.1.3
Digital Intra-oral X-ray Image Storage for Processing	1.2.840.10008.5.1.4.1.1.1.3.1
Digital Mamography X-ray Image Storage for Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital Mamography X-ray Image Storage for Processing	1.2.840.10008.5.1.4.1.1.1.2.1
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2
VL Slide Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4
Patient Root Find	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Move	1.2.840.10008.5.1.4.1.2.1.2
Study Root Find	1.2.840.10008.5.1.4.1.2.2.1
Study Root Move	1.2.840.10008.5.1.4.1.2.2.2
Patient Study Only Root Find	1.2.840.10008.5.1.4.1.2.3.1
Patient Study Only Root Move	1.2.840.10008.5.1.4.1.2.3.2

3.1.2. Query / Retrieve - Specification

Patterson DICOM Imaging provides Standard Conformance to the following DICOM 3.0 Standard SOP Class as a SCU.

Table 2. Query / Retrieve SOP Classes Supported by Patterson DICOM Imaging

SOP Class Name	SOP Class ID
Patient Root Find	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Move	1.2.840.10008.5.1.4.1.2.1.2
Study Root Find	1.2.840.10008.5.1.4.1.2.2.1
Study Root Move	1.2.840.10008.5.1.4.1.2.2.2
Patient Study Only Root Find	1.2.840.10008.5.1.4.1.2.3.1
Patient Study Only Root Move	1.2.840.10008.5.1.4.1.2.3.2

3.1.3. Verification - Specification

Patterson DICOM Imaging provides Standard Conformance to the following DICOM 3.0 Standard

SOP Class as a SCU.

Table 3. Verification SOP Class Supported by Patterson DICOM Imaging

SOP Class Name	SOP Class ID
Verification	1.2.840.10008.1.1

3.1.4. Association Establishment Policies for Patterson DICOM Imaging AE

3.1.4.1. General

All associations with Patterson DICOM Imaging are established using the DICOM 3.0 Standard application context.

1. Patterson DICOM Imaging initiates an association for verification.
2. Patterson DICOM Imaging initiates an association to query database.
3. Patterson DICOM Imaging initiates an association to send and store images.
4. Patterson DICOM Imaging initiates an association to transfer images.
5. Patterson DICOM Imaging accepts an association to receive and store images transferred by the C-Move SCP

3.1.4.2. Number of Associations

Only one instance of Patterson DICOM Imaging can be running at a time. Patterson DICOM Imaging opens only one association.

3.1.4.3. Asynchronous Nature

Not supported.

3.1.4.4. Implementation Identifying Information

Patterson Dental Supply, Inc. DICOM Imaging implementation provides a single Class Unique Identifier (CUID) -- 1.2.840.114257-- and a Version Name – Patterson Dental.

3.1.5. Association Initiation Policies for Patterson DICOM Imaging AE

3.1.5.1. Real World Activity: Request for Verification

3.1.5.1.1. Associated Real World Activity

Patterson DICOM Imaging initiates an association with the server to verify the current DICOM association

3.1.5.1.2. Presentation Contexts

Table 4. Presentation Contexts to Verify DICOM Association

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

3.1.5.2. Real World Activity: Request to Get Worklist / Query Database

3.1.5.2.1. Associated Real World Activity

Patterson DICOM Imaging initiates an association with Server to get the patient worklist or to send query requests and to receive the appropriate C-Find status code.

3.1.5.2.2. Presentation Contexts

Table 5. Presentation Contexts to Query Database

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Patient Root Query/Retrieve (Find)	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Study Root Query/Retrieve (Find)	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Patient/Study Only Query/Retrieve (Find)	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

3.1.5.3. Read World Activity: Request to Send and Store Images

3.1.5.3.1. Associated Real World Activity

Patterson DICOM Imaging initiates an association with the server to send and store images and to receive the appropriate C-Store status code.

3.1.5.3.2. Presentation Contexts

Table 6. Presentation Contexts to Send and Store Images

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Digital X-ray Image Storage (Presentation)	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed	1.2.840.10008.1.2.1	SCU	None
Digital Intra-oral X-ray Image Storage (Presentation)	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Little Endian Uncompressed	1.2.840.10008.1.2.1	SCU	None

3.1.5.4. Real World Activity: Request to Transfer Images

3.1.5.4.1. Associated Real World Activity

Patterson DICOM Imaging initiates an association with the server to transfer images and to issue the appropriate C-Move status code.

3.1.5.4.2. Presentation Contexts

Table 7. Presentation Contexts to Transfer Images

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Patient Root Query/Retrieve (Move)	1.2.840.10008.5.1.4.1.2.1.2	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Study Root Query/Retrieve (Move)	1.2.840.10008.5.1.4.1.2.2.2	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Patient/Study Only Query/Retrieve (Move)	1.2.840.10008.5.1.4.1.2.3.2	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None

3.1.6. Association Acceptance Policies for Patterson DICOM Imaging AE

3.1.6.1. Real World Activity: Respond to Store Images Request

3.1.6.1.1. Associated Real World Activity

Patterson DICOM Imaging accepts an association to store images as a result of a C-Move request.

3.1.6.1.2. Presentation Contexts

Table 8. Transfer Syntaxes to Store Images

Name	UID
Implicit VR Little Endian	1.2.840.10008.1.2
Explicit VR Little Endian	1.2.840.10008.1.2.1
Implicit VR Big Endian	1.2.840.10008.1.2.2
JPEG Baseline	1.2.840.10008.1.2.4.50
JPEG Extended	1.2.840.10008.1.2.4.51
JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
JPEG 2000	1.2.840.10008.1.2.4.91
RLE Lossless	1.2.840.10008.1.2.5

Table 9: Presentation Contexts to Store Images

Abstract Syntax		Transfer Syntax	Role	Extended Negotiation
Name	UID			
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	All from Table 8	SCP	None
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	All from Table 8	SCP	None
MR Image Storage	1.2.840.10008.5.1.4.1.4	All from Table 8	SCP	None
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	All from Table 8	SCP	None
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	All from Table 8	SCP	None
Ultrasound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	All from Table 8	SCP	None
X-ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	All from Table 8	SCP	None

X-ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	All from Table 8	SCP	None
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	All from Table 8	SCP	None
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	All from Table 8	SCP	None
Digital X-ray Image Storage (Presentation)	1.2.840.10008.5.1.4.1.1.1.1	All from Table 8	SCP	None
Digital X-ray Image Storage (Processing)	1.2.840.10008.5.1.4.1.1.1.1.1	All from Table 8	SCP	None
Digital Intra-oral X-ray Image Storage (Presentation)	1.2.840.10008.5.1.4.1.1.1.3	All from Table 8	SCP	None
Digital Intra-oral X-ray Image Storage (Processing)	1.2.840.10008.5.1.4.1.1.1.3.1	All from Table 8	SCP	None
Digital Mamography X-ray Image Storage (Presentation)	1.2.840.10008.5.1.4.1.1.1.2	All from Table 8	SCP	None
Digital Mamography X-ray Image Storage (Processing)	1.2.840.10008.5.1.4.1.1.1.2.1	All from Table 8	SCP	None
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	All from Table 8	SCP	None
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	All from Table 8	SCP	None
VL Slide Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	All from Table 8	SCP	None
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	All from Table 8	SCP	None

Communication Profiles

4.1. Supported Communication Stacks

Patterson DICOM Imaging provides TCP/IP Network Communication Support in accordance with DICOM 3.0 Standard.

4.2. TCP/IP Stack

Patterson DICOM Imaging communicates over the TCP/IP protocol stack on any physical interconnection supporting the TCP/IP stack.

4.3. Physical Media Support

Patterson DICOM Imaging is indifferent to the physical medium over which the TCP/IP executes.

Configuration

5.1. Configurable Settings

The following settings are configurable at the Patterson DICOM Imaging Configuration dialog box.

1. Remote IP Address
2. Remote Port Number
3. Remote Application Entity Title (Called AE)
4. Local Application Entity Title (Calling AE)
5. Local IP Address
6. Local Port Number